





FBI



2025 RELEASE UNDER E.O. 14176



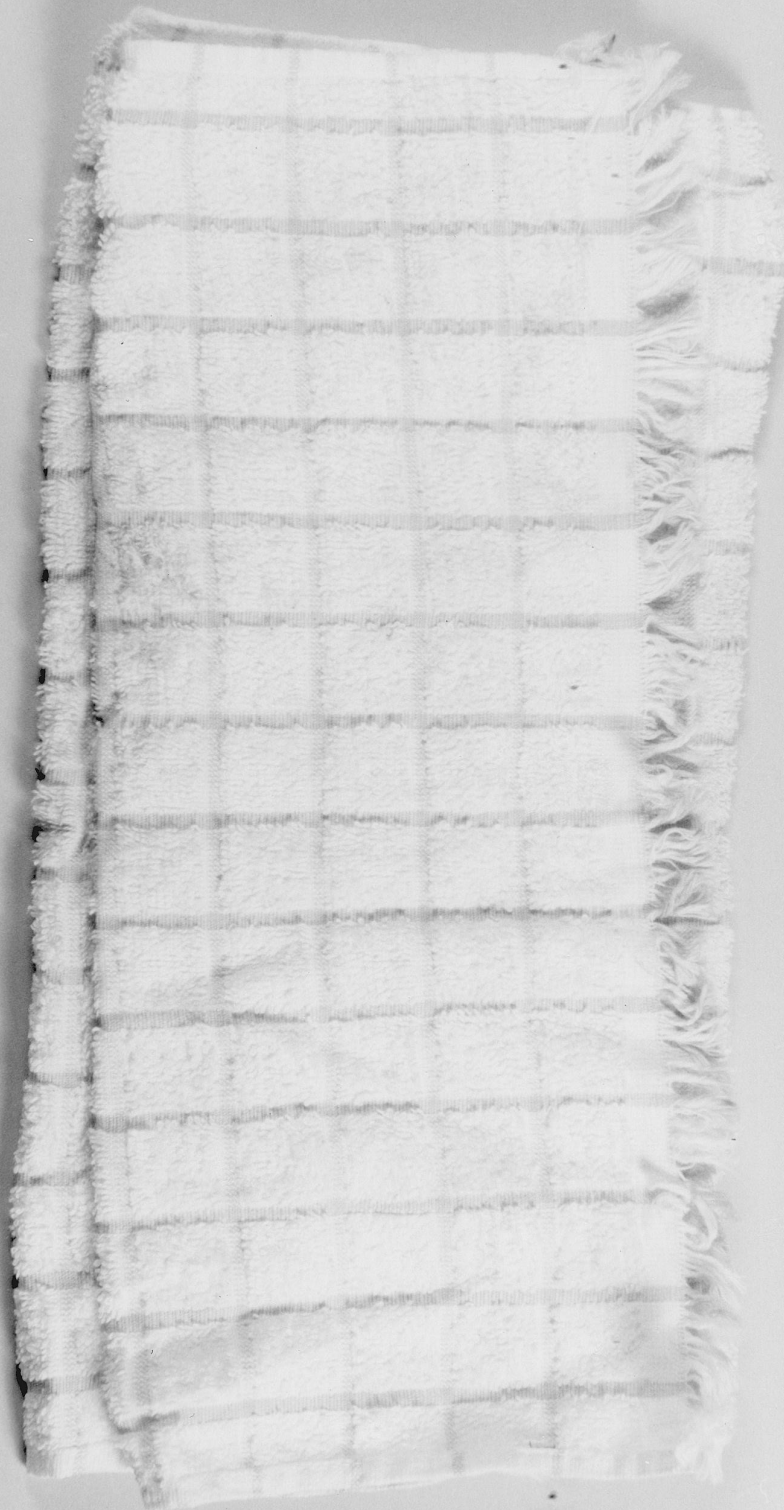


Q26
FBI
LABORATORY
PC-A5718 BX JV


GENIC
SU OF INVESTIGAT
NGTON, D. C.



EVI
FEDERAL B
W

Q27
FBI
LABORATORY
PC A5498 BX JV

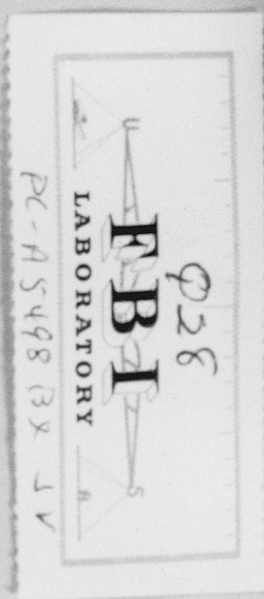

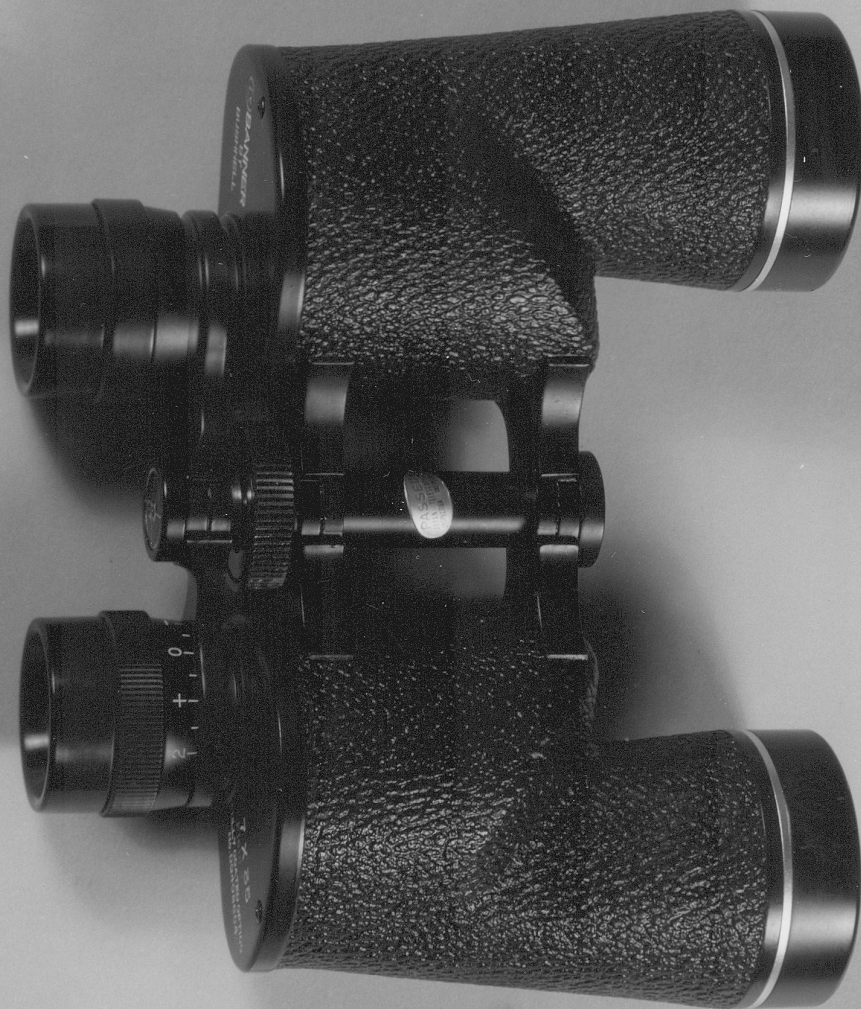


Q14
FBI
LABORATORY
PC-A5478 BX JV




2025 RELEASE UNDER E.O. 14176



2025 RELEASE UNDER E.O. 14176

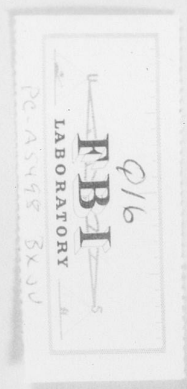



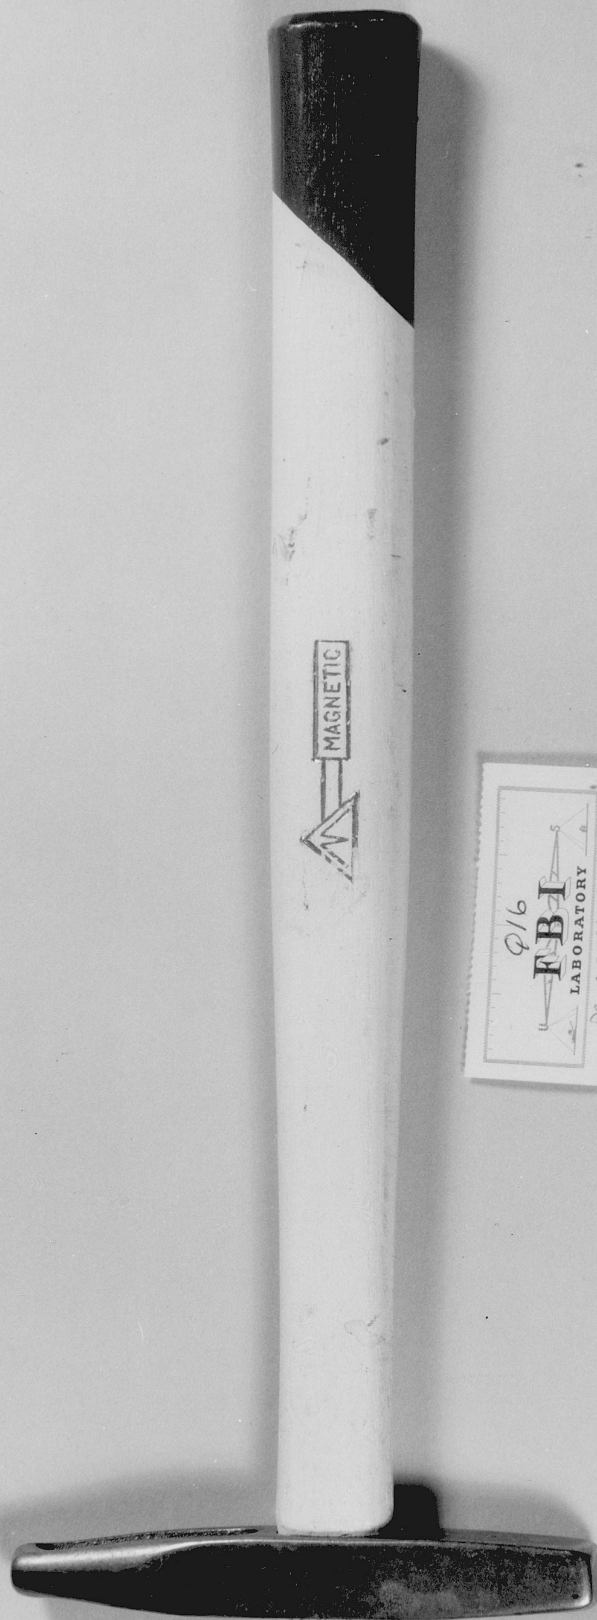



Q17
FBI
LABORATORY
PC-A5498 BX VV

31 ADHESIVE BANDAGES
21-3/4" STRIPS • 10 JUNIORS

BAND-AID
BRAND
**sheer
strips**





**NEW OVERALL AIR-VENTS
for faster healing**



Air-vents over the gauze pad—speed healing. Air-vents on the tape part keep the skin fresh. More comfortable to wear—with SUPER-STICK. For best results, be sure skin is clean and dry before applying bandage. Good medical practice suggests changing bandage if pad becomes wet.



Johnson & Johnson


NEW BRUNSWICK, NEW JERSEY • MADE IN U.S.A. • C.J.&J.
CODE 4614


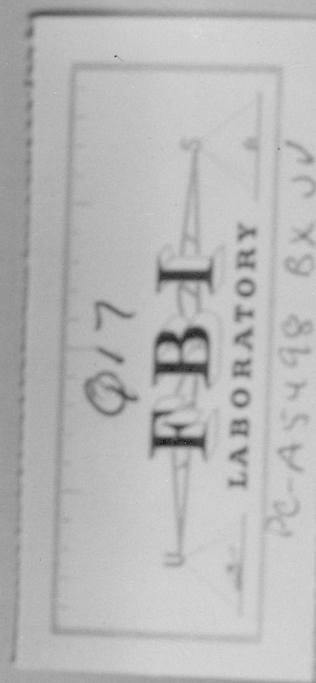


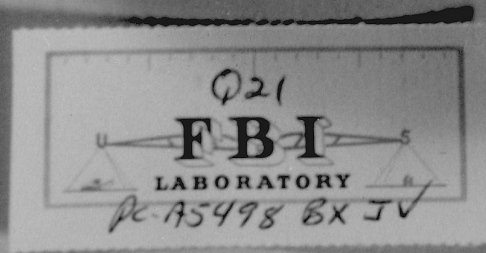

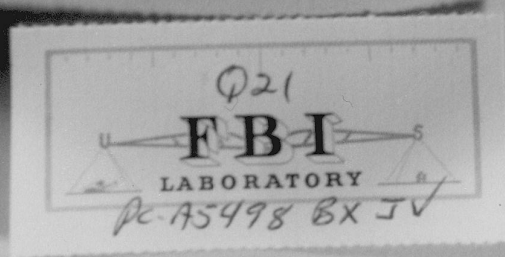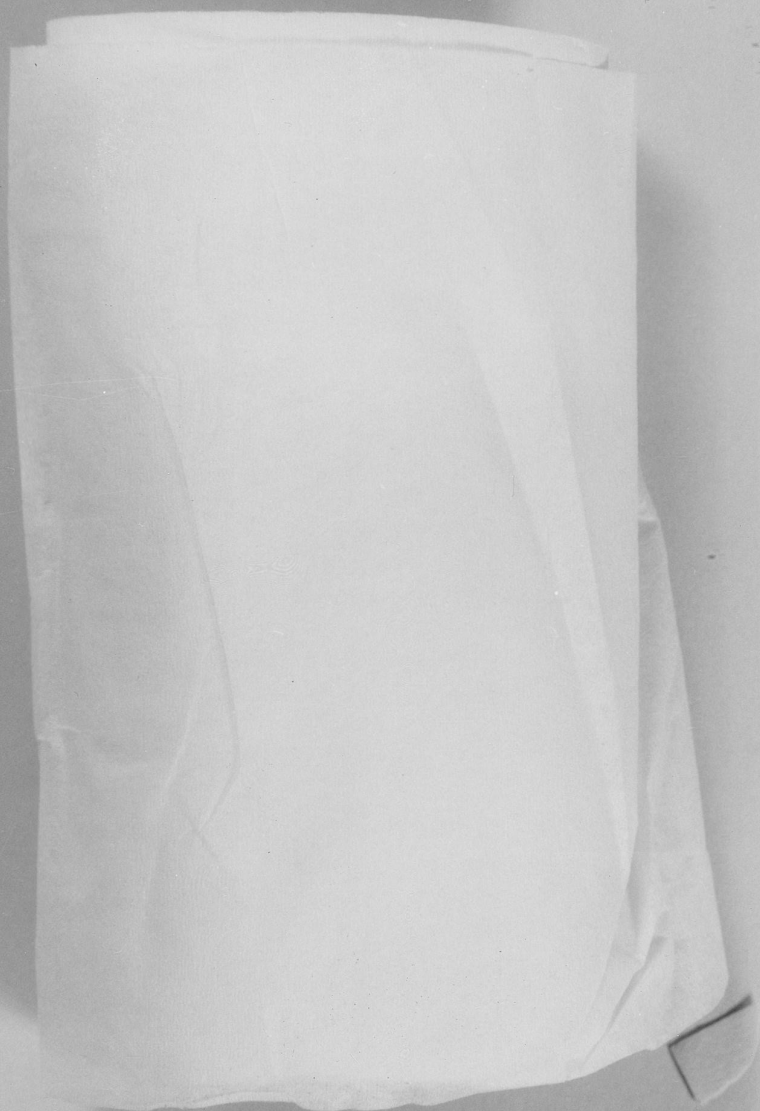


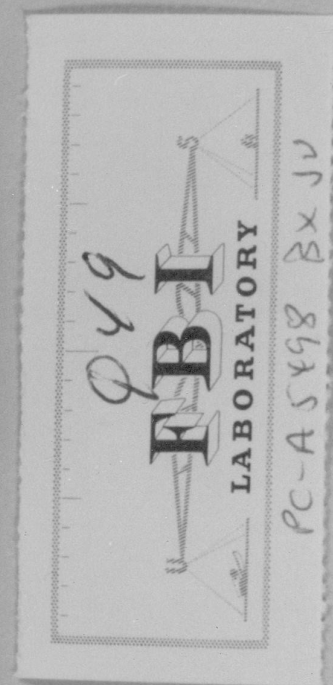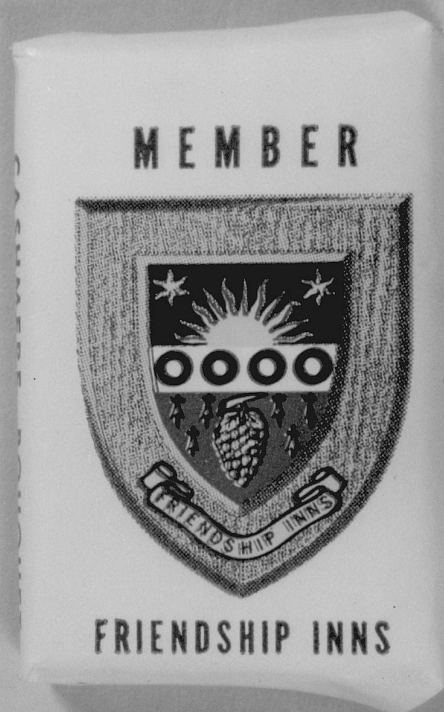



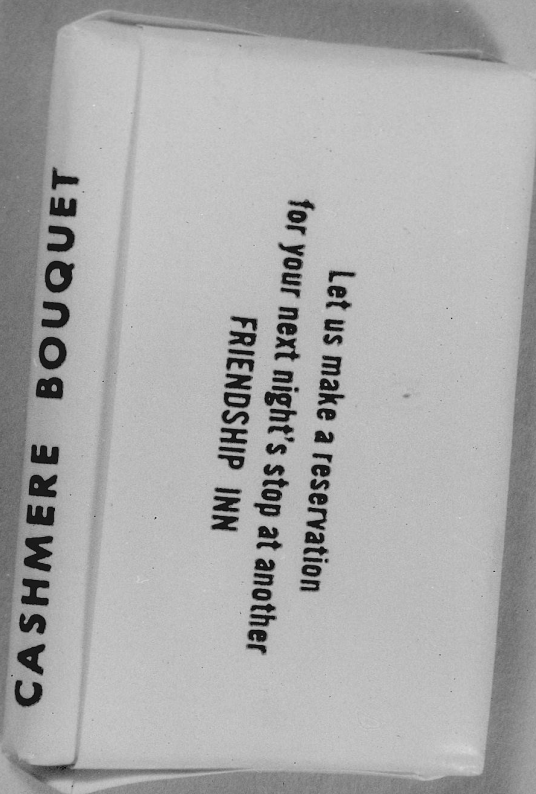


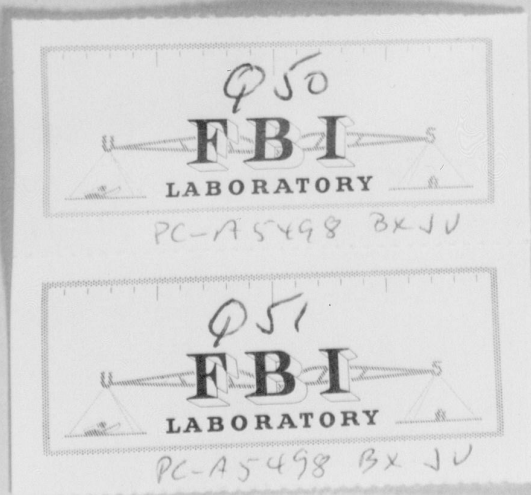




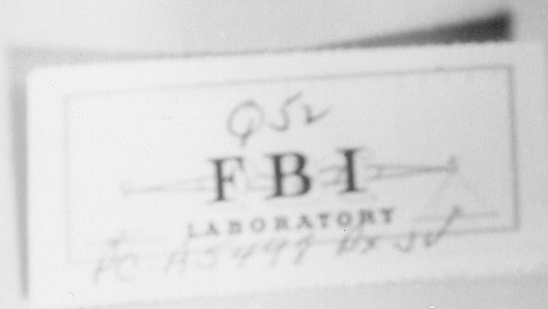

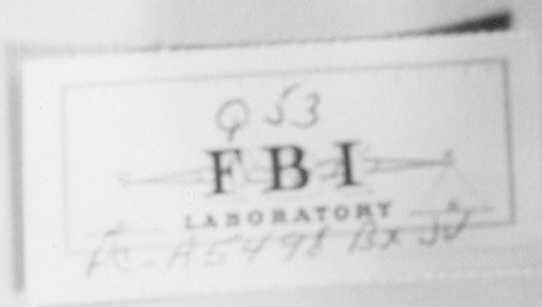

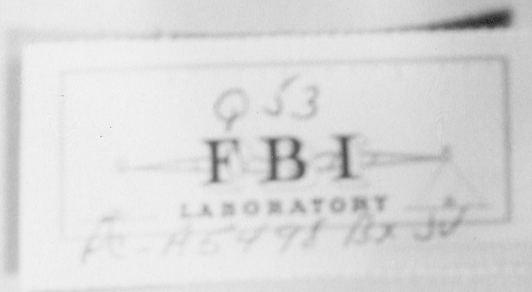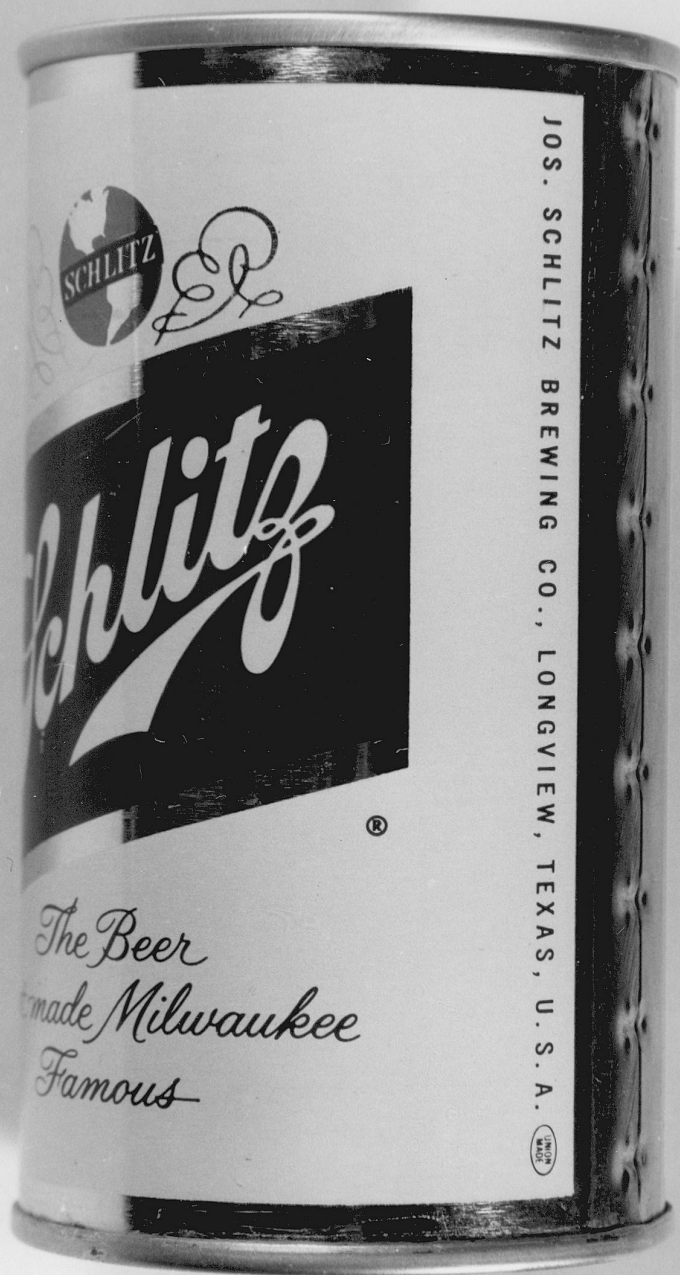



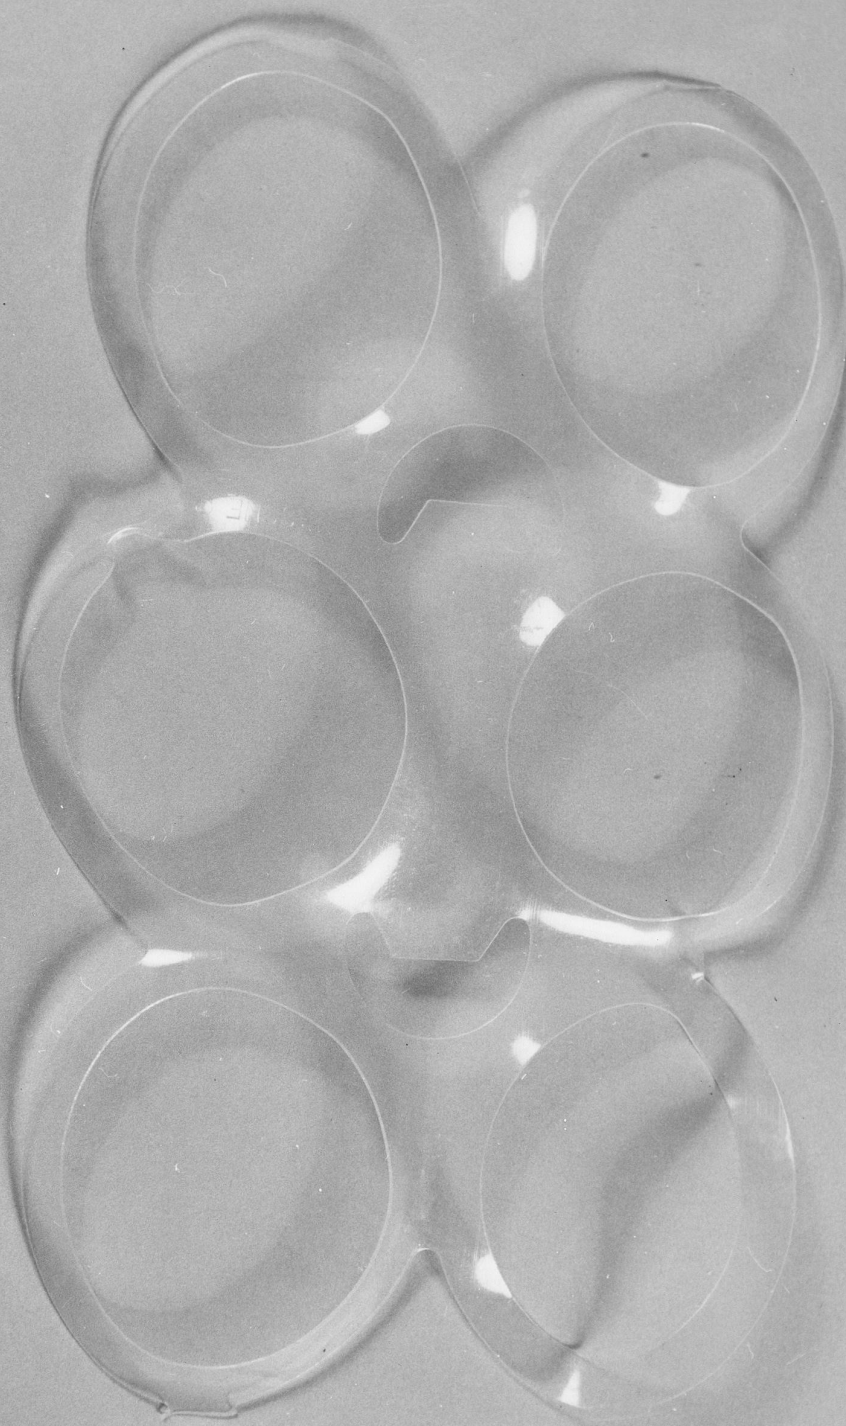

Q54
FBI
LABORATORY
PC-A5498 BX JV



FBI
LABORATORY
FBI

Q55



Q55
FBI
LABORATORY
PC-A5478 BK IV

Q55



2025 RELEASE UNDER E.O. 14176



2025 RELEASE UNDER E.O. 14176



2025 RELEASE UNDER E.O. 14176



2025 RELEASE UNDER E.O. 14176



2025 RELEASE UNDER E.O. 14176



Q14
— FBI —
LABORATORY
PC-A5498 BX JV

